
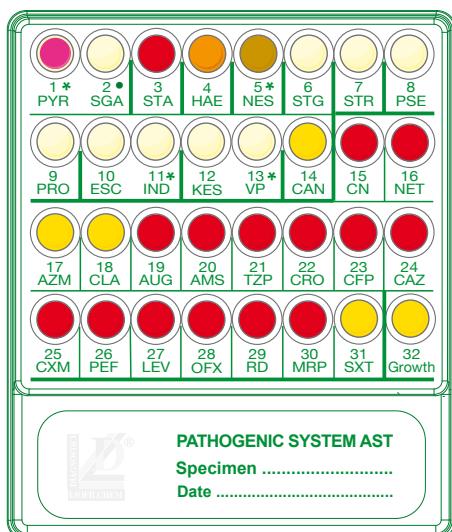
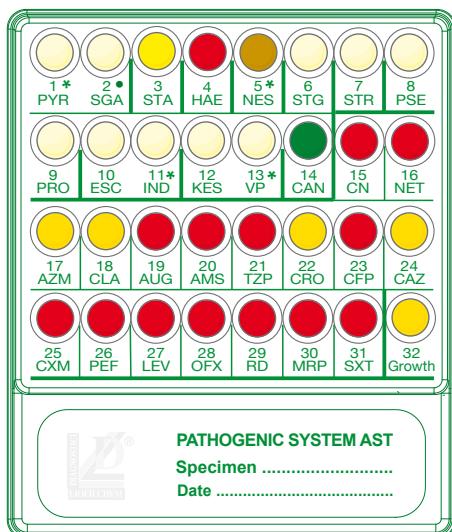


PATHOGENIC SYSTEM AST

Identification and Antimicrobial Susceptibility Testing of the main pathogenic microorganisms directly from Clinical Specimens

Liofilchem® and the Liofilchem company logo are registered trademarks of LIOFILCHEM s.r.l.

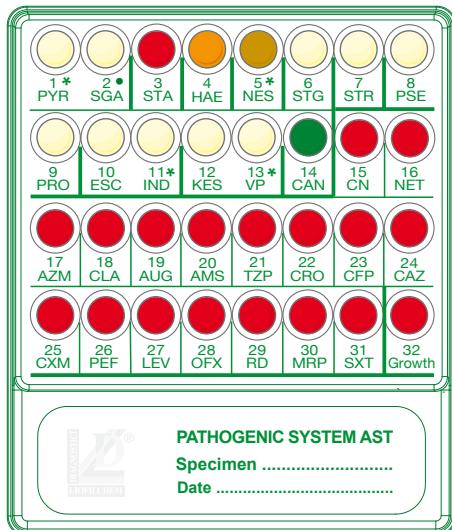

★ Clinical Specimens

Pharyngeal swab, Cutaneous swab,
Auricular swab, Ophthalmic swab,
Expectorate, Exudates and other clinical specimens.

★ Direct microbial identification

Streptococcus pyogenes (group A), *Staphylococcus aureus*,
Haemophylus spp., *Neisseria* spp., *Escherichia coli*,
Streptococcus agalactiae (group B),
Klebsiella spp., *Enterobacter* spp., *Serratia* spp.,
Proteus spp., *Providencia* spp., *Pseudomonas* spp.,
Enterococcus spp. (group D), *Candida* spp.

★ Antimicrobial Susceptibility Testing

Gentamicin, Netilmicin, Azithromycin, Clarithromycin,
Amoxicillin-Clavulanic Acid, Ampicillin-Sulbactam,
Piperacillin-Tazobactam, Ceftriaxone, Cefoperazone,
Ceftazidime, Cefuroxime, Pefloxacin, Levofloxacin,
Ofloxacin, Rifampicin, Meropenem, Co-trimoxazole.










★ Benefits

- ✓ Complete diagnosis
- ✓ Save time and labor with direct testing
- ✓ Results in 18-24 hours
- ✓ Confirmation with latex agglutination tests
- ✓ Clear and well defined color changes
- ✓ Easy interpretation

PATHOGENIC SYSTEM AST

RESULTS

Identification



Antimicrobial Susceptibility Testing



Sensitivity

Resistance

Liofilchem® and the Liofilchem company logo are registered trademarks of LIOFILCHEM s.r.l.

DESCRIPTION	PACKAGING	REF.
PATHOGENIC SYSTEM AST	20 tests	71681
OXIDASE TEST STICK	30 tests	88029
STREPTO A LATEX KIT	50 tests	96154
STREPTO B LATEX KIT	50 tests	96153
STAPH LATEX KIT	50 tests	96017

TEST PROCEDURE



- Dip the clinical specimen into a tube of nutrient broth and incubate at 36±1°C for 2-3 hours.



- Transfer 0.2 mL of culture broth into the vial of Physiological Solution (**Suspension A**).
- Transfer 0.01 mL of culture broth into the vial of Inoculum Broth 2 (**Suspension B**).



- Add a Pyr Disc into the well 1-PYR.
- Add 0.2 mL of the **Suspension A** into each well from 1 to 14. (**Identification**)



- Add 0.2 mL of the **Suspension B** into each well from 15 to 32. (**Antimicrobial Susceptibility Testing**)
- Incubate at 36±1°C for 18-24 h.



- Confirm the presence of:
 - Streptococcus pyogenes* (group A)
 - Staphylococcus aureus*
 - Haemophilus* spp.
 - Neisseria* spp.
 - Streptococcus agalactiae* (group B)
 as by Instruction For Use.



- Confirm *Candida* spp. by taking a drop from the positive well 14-CAN and watch for spores at the microscope (400x).
- Note down the test results on the form provided in the kit, or read and interpret by **automatic readers**.