

# Thermo Scientific™ Listeria PreciS™ Methods

Publication Number MAN0026538 Revision G



**WARNING!** Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves. Safety Data Sheets (SDSs) are available from [thermofisher.com/support](https://www.thermofisher.com/support).

## Intended use

Thermo Scientific™ Oxoid™ *Brilliance*™ Listeria Agar (ISO) complies with the formulation described by Ottaviani and Agosti (see “References” on page 20).

- Thermo Scientific™ Listeria PreciS™ Detection Method allows the simultaneous detection of presumptive positive samples for *Listeria* species and *L. monocytogenes* within two days. The method enables negative products to be released at least 24 hours earlier than the reference methods.
- Thermo Scientific™ Listeria PreciS™ Enumeration Method allows the enumeration of *Listeria* species and *L. monocytogenes* within two days. The method enables negative products to be released at least 24 hours earlier than the reference methods.

Flexibility is offered with the possible use of (1) two enrichment broths in the detection workflow, (2) surface and pour plating in the enumeration workflow, and (3) multiple confirmations. Note that it is possible to confirm presumptive results the same day or the next day after the recovery of characteristic colonies.

Both detection and enumeration workflows are meant for use in laboratories undertaking microbiological analysis.

## Summary

Oxoid™ *Brilliance*™ Listeria Agar (ISO) is a chromogenic medium incorporating X-glucoside. This chromogen is cleaved by the enzyme beta-glucosidase, common to all *Listeria* species, giving rise to blue-green colonies. Other organisms that are positive for this enzyme are inhibited by the selective agents in the medium: lithium chloride, polymyxin B, ceftazidime, and nalidixic acid. Inclusion of amphotericin inhibits the growth of any yeasts and molds present. *Listeria monocytogenes* colonies are then further differentiated by their ability to produce the phospholipase enzymes PIPLC and PCPLC which hydrolyse phosphatidylinositol or lethicin in the medium, producing an opaque white halo around the colony. Note that some pathogenic *L. ivanovii* strains can also produce halos, but these halos are smaller than the halos around *L. monocytogenes* colonies.

The *Listeria* *Precis*™ Detection Method combines the benefits of one single enrichment to the benefit of Oxoid™ *Brilliance*™ *Listeria* chromogenic Agar (ISO). Simply streak 10 µL of the enrichment broth on the Oxoid™ *Brilliance*™ *Listeria* chromogenic Agar (ISO) using a basic inoculation loop, with no need of pipetting a higher volume.

The *Listeria* *Precis*™ Detection Method offers two enrichment broth options—the Thermo Scientific™ Oxoid™ ONE Broth–*Listeria* and the Thermo Scientific™ Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB).

This method reduces the time to result over standard culture methods for both negative and positive screening.

The *Listeria* *Precis*™ Enumeration Method offers flexibility and ease-of-use. Surface and pour plating can be run to facilitate the handling depending on the contamination levels.

The confirmation procedures can be performed on isolated characteristic colonies without the need of a purification step. Same-day results can be generated thanks to the Thermo Scientific™ *PrecisCheck*™ *L. monocytogenes* Kit and Thermo Scientific™ *PrecisCheck*™ *Listeria* species Kit, the Thermo Scientific™ Oxoid™ Biochemical Identification System (O.B.I.S.) Mono, the Thermo Scientific™ *SureTect*™ *Listeria* species PCR Assay, or the Thermo Scientific™ *SureTect*™ *Listeria* *monocytogenes* PCR Assay (or equivalent) as described in the ISO 7218:2007 standard. The use of the Thermo Scientific™ Oxoid™ *Microbact*™ *Listeria* 12L Kit (or equivalent) or Rhamnose test provides next-day results. It is as well possible to use any appropriate ISO 16140-6:2019 validated confirmation methods or any appropriate reference confirmation procedure (e.g. ISO 11290-1:2017, FDA BAM Chapter 10, USDA/FSIS MLG 8.13).

## Media composition

Unless otherwise indicated, all materials are available through [thermofisher.com](http://thermofisher.com). "MLS" indicates that the material is available from [fisherscientific.com](http://fisherscientific.com) or another major laboratory supplier.

The following compositions are for typical formulae. Adjustments might be required to meet performance standards.

**Table 1** Thermo Scientific™ Oxoid™ ONE Broth–*Listeria* Base (Cat. No. [CM1066B](#) 500 g, [CM1066R](#) 2.5 kg)

Reagents	Concentration
Peptone	28.0 g/L
Salt mix	10.0 g/L
Carbohydrate mix	6.0 g/L (anhydrous)
pH 7.4 ± 0.2 at 25°C	

**Table 2** Thermo Scientific™ Oxoid™ ONE Broth–*Listeria* Selective Supplement (Cat. No. [SR0234B](#) 10 vials each for 2.25 L, [SR0234E](#) 10 vials each for 500 mL)

Reagents	Concentration
The formulation of Oxoid™ ONE Broth– <i>Listeria</i> Selective Supplement is not published.	

**Table 3 Thermo Scientific™ Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Base (Cat. No. [CM1107B](#))**

Reagents	Concentration
Peptone	23.4 g/L
Yeast extract	5.0 g/L
Lithium chloride	10.0 g/L
Ferric ammonium citrate	0.1 g/L
Sodium chloride	5.0 g/L
pH 7.4 ± 0.2 at 25°C	

**Table 4 Thermo Scientific™ Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Selective Supplement (Cat. No. [SR0243E](#))**

Vial contents	<a href="#">SR0243E</a> (1 vial per 500 mL medium)	Per litre before sample addition
Polymyxin	5.0 mg	10.0 mg
Quinolone antimicrobials	17.5 mg	35.0 mg

**Table 5 Thermo Scientific™ Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Complete (Cat. No. [CM1154B](#))**

Reagents	Concentration
Peptone	23.4 g/L
Yeast extract	5.0 g/L
Lithium chloride	10.0 g/L
Ferric ammonium citrate	0.1 g/L
Sodium chloride	5.0 g/L
Polymyxin	10.0 mg
Quinolone antimicrobials	35.0 mg
pH 7.4 ± 0.2 at 25°C	

**Table 6 Thermo Scientific™ Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB) Buffer Supplement (Cat. No. [BO1339E](#); [BO1204M](#))**

Item	Source
Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB) Buffer Supplement <sup>[1]</sup> <ul style="list-style-type: none"> <li>• 24 × 10 mL</li> <li>• 10 × 100 mL</li> </ul>	<p><a href="#">BO1339E</a></p> <p><a href="#">BO1204M</a></p> <p>Available through the Thermo Fisher Microbiology ordering process</p>

<sup>[1]</sup> This product may crystallize during storage. If crystals are present, place the tube in a 37°C water bath for 5–10 minutes, or until all of the crystals are dissolved.

**Table 7 Thermo Scientific™ Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Base (Cat. No. [CM1212](#))**

Reagents	Concentration
Enzymatic digest of animal tissues	18.0 g/L
Enzymatic digest of casein	6.0 g/L
Yeast extract	10.0 g/L
Sodium pyruvate	2.0 g/L
Glucose	2.0 g/L
Magnesium glycerophosphate	1.0 g/L
Magnesium sulphate (anhydrous)	0.5 g/L
Sodium chloride	5.0 g/L
Lithium chloride	10.0 g/L
Disodium hydrogen phosphate (anhydrous)	2.5 g/L
5-Bromo-4-chloro-3-indolyl-β-d-glucopyranoside	0.05 g/L
Agar	12.0 g/L
pH 7.2 ± 0.2 at 25°C	

**Table 8 Thermo Scientific™ Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Selective Supplement (Cat. No. [SR0257E](#); [SR0257B](#))**

Typical formulation	<a href="#">SR0257E</a> (1 vial per 500 mL medium)	<a href="#">SR0257B</a> (1 vial per 200 mL <a href="#">BO1370Z</a> medium)	Per litre
Nalidixic acid sodium salt	10.0 mg	4.0 mg	20.0 mg
Polymyxin B sulphate	38,350 IU	15,340 IU	76,700 IU
Ceftazidime	10.0 mg	4.0 mg	20.0 mg
Amphotericin B	5.0 mg	2.0 mg	10.0 mg

**Table 9** Thermo Scientific™ Oxoid™ *Brilliance*™ Listeria Agar (ISO) Differential Supplement (Cat. No. SR0258E; SR0258B)

Typical formulation	SR0258E (1 vial per 500 mL medium)	SR0258B (1 vial per 200 mL BO1370Z)	Per litre
L-α-phosphatidylinositol solution	15.0 mL	6.0 mL	30.0 mL

**Table 10** Thermo Scientific™ Oxoid™ prepared media and other media

Item	Source
Oxoid™ ONE Broth–Listeria Base in Bottles (10 × 225 mL)	BO1066S <sup>[1]</sup>
Oxoid™ ONE Broth–Listeria Base in Ready Bags (3 × 3 L)	FR60031 <sup>[1]</sup>
Oxoid™ <i>Brilliance</i> ™ Listeria Agar (ISO) (10 ready-to-use 90 mm plates)	PO1298A <sup>[1]</sup> or PO5332A <sup>[1]</sup>
Oxoid™ <i>Brilliance</i> ™ Listeria Agar (ISO) (10 × 200 mL bottles)	BO1370Z <sup>[1]</sup> SR0257B <sup>[1]</sup> SR0258B <sup>[1]</sup>
Oxoid™ 24 Listeria Enrichment Broth (24 LEB) (10 × 225 mL in 250 mL PET sirop bottles)	BO1205S <sup>[1,2]</sup>
Oxoid™ 24 LEB Complete (Oxoid™ 24 Listeria Enrichment Broth (24 LEB) (Dehydrated) plus Oxoid™ 24 LEB Selective Supplement)	CM1154B
Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Buffer Supplement <sup>[3]</sup> <ul style="list-style-type: none"> <li>• 24 × 10 mL</li> <li>• 10 × 100 mL</li> </ul>	BO1339E BO1204M
Oxoid™ Buffered Peptone Water ISO Formulation, Dehydrated	CM1211B, CM1049B, or equivalent
Thermo Scientific™ FitBag™ 24 Listeria Enrichment Broth <ul style="list-style-type: none"> <li>• 30 × 2.7 L</li> <li>• 20 × 4.5 L</li> <li>• 10 × 9 L</li> </ul>	DF1107A DF1107B DF1107C
Thermo Scientific™ QuickBag™ 24 Listeria Enrichment Broth <ul style="list-style-type: none"> <li>• 3 × 2.7 L</li> <li>• 2 × 4.5 L</li> </ul>	DQ1107A DQ1107B
Thermo Scientific™ Dry-Bags™ 24 Listeria Enrichment Broth (5 × 20 L)	DB1107V

<sup>[1]</sup> Check code and availability with your local Oxoid™ Representative.

<sup>[2]</sup> Includes 24 LEB Selective Supplement (SR0243E). Do not use in the Listeria PreciS™ Enumeration Method.

<sup>[3]</sup> This product may crystallize during storage. If crystals are present, place the tube in a 37°C water bath for 5–10 minutes, or until all of the crystals are dissolved.

**Table 11** Materials for confirmation testing

Item	Source
Thermo Scientific™ <i>PrecisCheck</i> ™ <i>L. monocytogenes</i> Kit	<a href="#">LF0200A</a>
Thermo Scientific™ <i>PrecisCheck</i> ™ <i>Listeria</i> species Kit	<a href="#">LF0100A</a>
Thermo Scientific™ <i>Oxoid</i> ™ Biochemical Identification System (O.B.I.S.) Mono	<a href="#">ID0600M</a>
Thermo Scientific™ <i>Oxoid</i> ™ <i>Microbact</i> ™ <i>Listeria</i> 12L Kit	<a href="#">MB1128A</a>
Thermo Scientific™ <i>SureTect</i> ™ <i>Listeria monocytogenes</i> PCR Assay	<a href="#">A56843</a>
Thermo Scientific™ <i>SureTect</i> ™ <i>Listeria</i> species PCR Assay	<a href="#">A56842</a>

## Required materials not supplied

- Inoculating loops, swabs, collection containers
- Incubators
- Quality control organisms

## Prepare the materials

---

**Note:** Ready-to-use Thermo Scientific™ *Oxoid*™ prepared media can be used as well. See Table 10.

---

### Prepare the *Oxoid*™ ONE Broth–*Listeria*

1. Suspend 22 g of *Oxoid*™ ONE Broth–*Listeria* Base (Cat. No. [CM1066](#)) in 500 mL (44 g/L) of distilled water.
2. Mix well, then sterilize by autoclaving at 121°C for 15 minutes.
3. Cool the medium to below 50°C.
4. Aseptically, add the contents of one vial of *Oxoid*™ ONE Broth–*Listeria* Selective Supplement (Cat. No. [SR0234E](#)), reconstituted as directed.

## Prepare the Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB)

1. Completely dissolve 21.75 g of Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB) Base (Cat. No. [CM1107B](#)) per 500 mL of distilled water.
2. Sterilize by autoclaving at 121°C for 15 minutes.
3. Cool to 50°C.
4. Aseptically, add the contents of one vial of Oxoid™ 24 LEB Selective Supplement (Cat. No. [SR0243E](#)) per 500 mL medium, reconstituted as directed.
5. Cool to room temperature before use.  
Store the prepared medium at 2–8°C in the dark.

## Prepare the Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB) Complete

1. Completely dissolve 43.5 g of Oxoid™ 24 LEB Complete (Cat. No. [CM1154B](#)) in 1,000 mL of distilled water.
2. Mix well, then sterilize by autoclaving at 121°C for 15 minutes.
3. Cool to room temperature (23±5°C) before use.  
Once made, store out of direct sunlight.

## Prepare the Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Base

1. Suspend 34.5 g of Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Base (Cat. No. [CM1212](#)) in 480 mL of distilled water.
2. Mix well and sterilize by autoclaving at 121°C for 15 minutes.
3. Cool the medium to 46°C.
4. Add one vial of Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Selective Supplement (Cat. No. [SR0257E](#)), reconstituted as directed, then add one vial of Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) Differential Supplement (Cat. No. [SR0258E](#)).
5. Mix well and pour into sterile petri dishes.

## Prepare the Oxoid™ *Brilliance*™ Listeria Agar (ISO) Bottle Media

1. Place the bottles containing 200 mL Oxoid™ *Brilliance*™ Listeria Agar (ISO) Base (Cat. No. [BO1370Z](#)) in a steamer for approximately 40–45 minutes to completely melt the agar until fully liquified.
2. Cool and maintain the molten agar in a water bath at  $46\pm 2^{\circ}\text{C}$ .
3. Aseptically supplement each bottle with 1 vial of Oxoid™ *Brilliance*™ Listeria Agar (ISO) Selective Supplement (Cat. No. [SR0257B](#)), reconstituted as directed, then add one vial of Oxoid™ *Brilliance*™ Listeria Agar (ISO) Differential Supplement (Cat. No. [SR0258B](#)).
4. Thoroughly mix the supplements with the molten agar by capping the bottle, then gently invert 2 or 3 times until the colour is homogeneous.
5. After melting and/or supplementation, the molten agar can be maintained in the water bath at  $44\text{--}46^{\circ}\text{C}$  for up to 4 hours, after which time the media must be discarded.

## Isolate *Listeria* species and *L. monocytogenes* from a broad range of foods and from environmental samples

Method certified EN ISO 16140-2:2016 by NF VALIDATION™ Certificate UNI 03/04-04/05 and UNI 03/14-06/22

Comply with Good Laboratory Practices (see EN ISO 7218:2007 standard).

The EN ISO 6887 series and the ISO 11290-1:2017 standard technical rules are optional for the preparation of the initial suspensions.

### 1. Enrich the samples as follows:

Matrices	Media	Incubation
25 g food samples	Prepare 1-in-10 ratio of sample to media. <ul style="list-style-type: none"> <li>Add up to 25 g of sample to 225 mL of Oxoid™ ONE Broth–<i>Listeria</i><sup>[1]</sup></li> <li>or</li> <li>Add up to 25 g of sample to 225 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB). Then add 10 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB) Buffer Supplement<sup>[2]</sup>.</li> </ul>	30±1°C for 25±3 hours for the supplemented Oxoid™ ONE Broth– <i>Listeria</i>
		37±1°C for 23±3 hours for the supplemented Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB)
Environmental samples	Prepare 1-in-10 ratio of sample to media. <ul style="list-style-type: none"> <li>Add up to 25 g of sample to 225 mL of Oxoid™ ONE Broth–<i>Listeria</i></li> <li>Add one swab to 10 mL of Oxoid™ ONE Broth–<i>Listeria</i></li> <li>Add one sponge to 100 mL of Oxoid™ ONE Broth–<i>Listeria</i></li> </ul>	30±1°C for 25±3 hours
	Prepare 1-in-10 ratio of sample to media. <ul style="list-style-type: none"> <li>Add up to 25 g of sample to 225 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB). Then add 10 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB) Buffer Supplement<sup>[2]</sup>.</li> <li>Add one swab to 10 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB). Then add 0.44 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB) Buffer Supplement<sup>[2]</sup>.</li> <li>Add one sponge to 100 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB). Then add 4.4 mL of Oxoid™ 24 <i>Listeria</i> Enrichment Broth (24 LEB) Buffer Supplement<sup>[2]</sup>.</li> </ul>	37±1°C for 23±3 hours

<sup>[1]</sup> ISO 16140-2:2016 validation scope restricted to selected food categories for *Listeria* spp. detection, i.e. meat products, dairy products, vegetables, fish, and seafood.

<sup>[2]</sup> This product may crystallize during storage. If crystals are present, place the tube in a 37°C water bath for 5–10 minutes, or until all of the crystals are dissolved.

2. (Optional) Store enrichment broths or plates after incubation at  $5\pm 3^{\circ}\text{C}$  for up to 72 hours before streaking or reading.
3. Gently agitate the bag, then, using a microbiological loop, inoculate a 10  $\mu\text{L}$  loopful of the broth onto a plate of Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) using a diminishing sweep technique to produce single colonies.
4. Incubate the plates at  $37\pm 1^{\circ}\text{C}$  as described for  $24\pm 2$  hours when using Oxoid™ ONE Broth–*Listeria* and at  $37\pm 1^{\circ}\text{C}$  for  $24\pm 2$  hours when using Oxoid™ 24 *Listeria* Enrichment Broth (24 LEB) (except for meat products when enriched in Oxoid™ ONE Broth–*Listeria*).

---

**Note:** For meat samples enriched in Oxoid™ ONE Broth–*Listeria*, re-incubate the plates that show no blue-green colonies at  $37\pm 1^{\circ}\text{C}$  for  $24\pm 2$  hours.

---

*Listeria* species colonies grow as blue-green colonies. *Listeria monocytogenes* colonies will include the addition of a typical halo. Non-target organisms are either inhibited or grow as straw or white colonies.

---


**Note:** Some *L. ivanovii* strains can as well show a typical halo due to a positive lecithinase activity, but these halos are smaller than the halos around *L. monocytogenes* colonies.

---

Blue-green colonies are presumptive positive *Listeria* species, and blue-green colonies with halos are presumptive positive *L. monocytogenes*.

See “Confirm positive results” to confirm the observed characteristic colonies.

## Listeria *Precis*™ Detection Method workflow

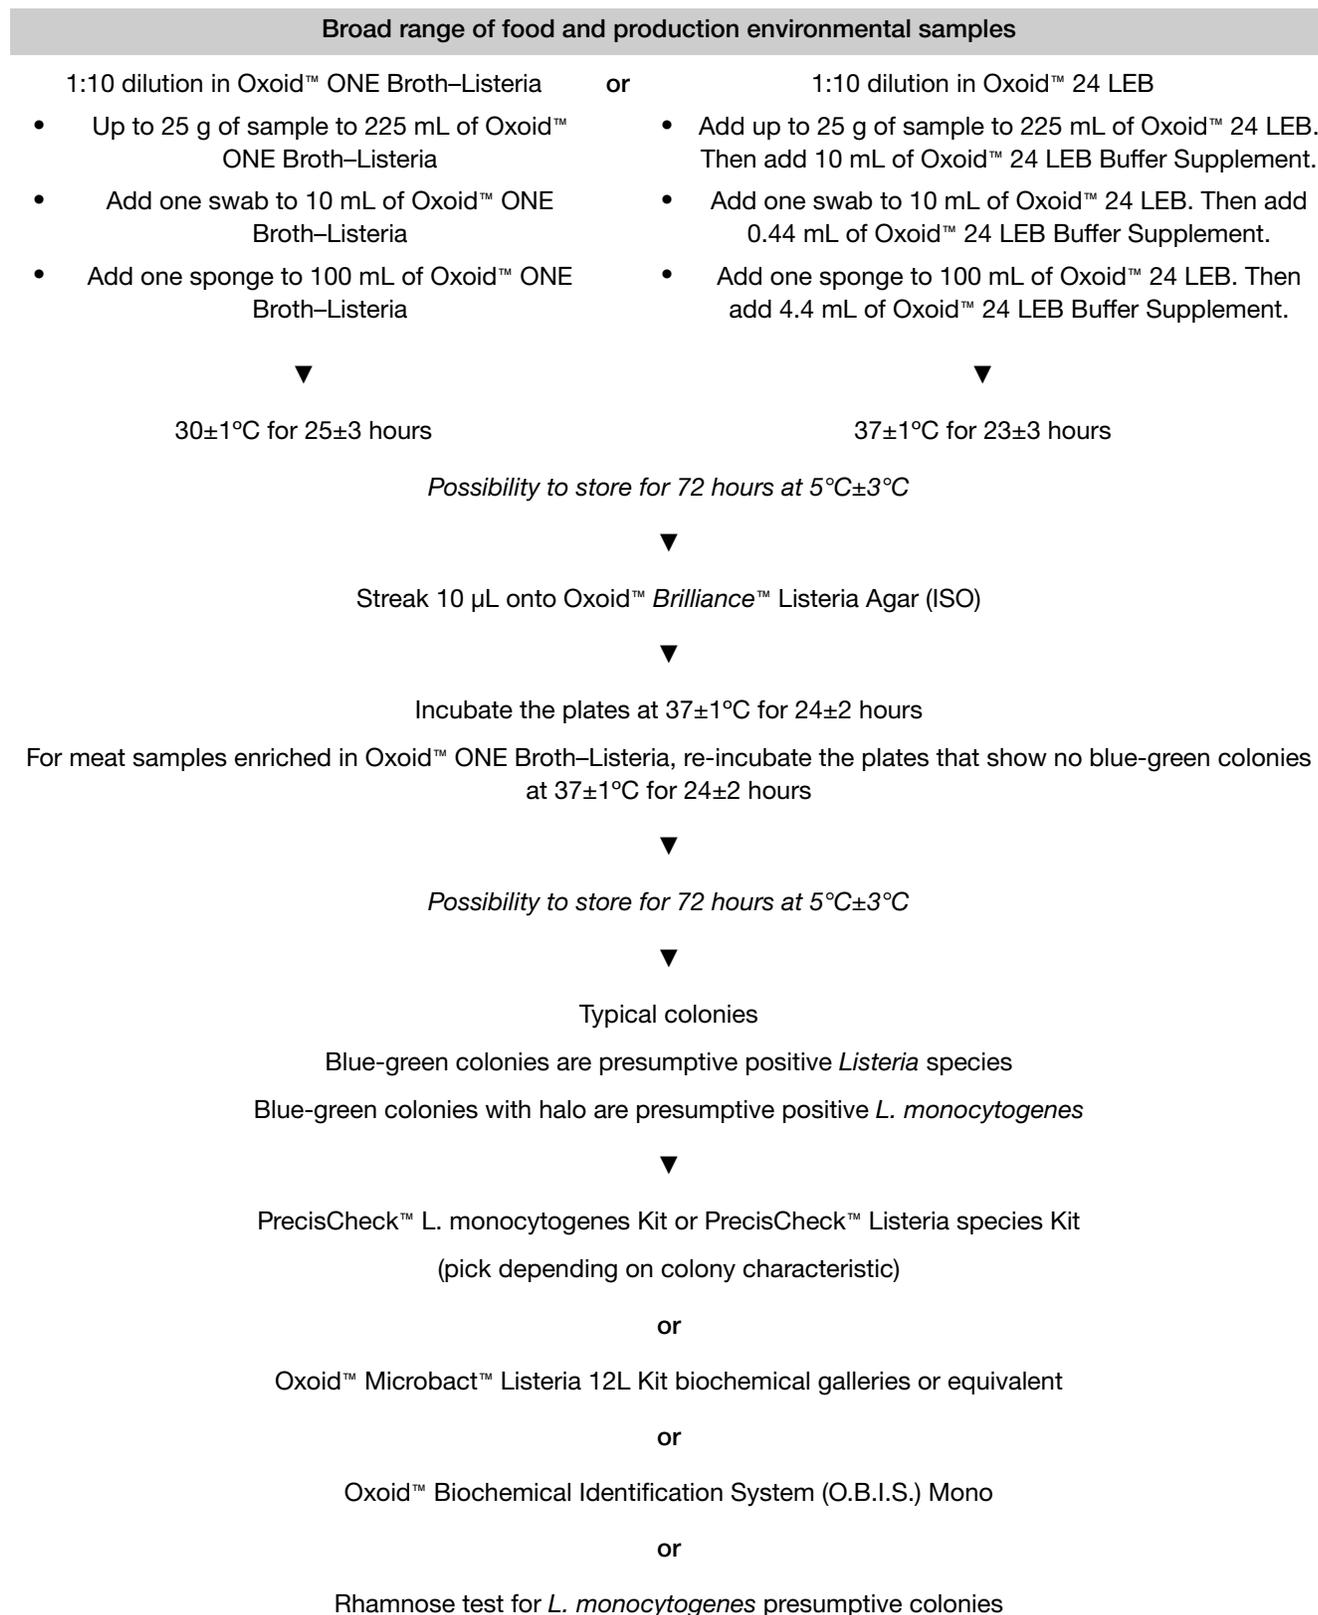

(continued)

**Broad range of food and production environmental samples**

or

EN ISO 11290-1:2017 confirmation procedure

or

Spot on Oxoid™ PALCAM for *Listeria* spp. presumptive colonies

or

Molecular hybridization test as described in EN ISO 7218:2007 (e.g. SureTect™ *Listeria* species PCR Assay and/or SureTect™ *Listeria monocytogenes* PCR Assay)

or

Any appropriate EN ISO 16140-6:2019 validated confirmation method (or any equivalent reference method procedure, e.g. FDA BAM, USDA/FSIS)

## Enumerate *Listeria* species and *L. monocytogenes* from a broad range of foods and from environmental surfaces

Method certified EN ISO 16140-2:2016 by NF VALIDATION™ Certificate UNI 03/04-09/06

Comply with Good Laboratory Practices (see EN ISO 7218:2007 standard).

For preparation of initial suspensions, it is recommended to follow the instructions of EN ISO 6887 series and EN ISO 11290-2:2017 standard.

1. Dilute the samples as follows:

Matrices	Media
10 g or 10 mL food samples and environmental samples	<ul style="list-style-type: none"> <li>Follow EN ISO 6887 series instructions and ISO 11290-2:2017 or</li> <li>1-in-10 ratio of sample to Oxoid™ 24 LEB (without selective supplement) with 4 mL of Oxoid™ 24 LEB Buffer Supplement<sup>[1]</sup></li> </ul>
25 g or 25 mL food samples and environmental samples	<ul style="list-style-type: none"> <li>Follow EN ISO 6887 series instructions and ISO 11290-2:2017 or</li> <li>1-in-10 ratio of sample to Oxoid™ 24 LEB (without selective supplement) with 10 mL of Oxoid™ 24 LEB Buffer Supplement<sup>[1]</sup></li> </ul>
Swab	<ul style="list-style-type: none"> <li>Follow EN ISO 6887 series instructions and ISO 11290-2:2017 or</li> <li>Add one swab to 10 mL Oxoid™ 24 LEB (without selective supplement) with 0.44 mL of Oxoid™ 24 LEB Buffer Supplement<sup>[1]</sup></li> </ul>
Sponge	<ul style="list-style-type: none"> <li>Follow EN ISO 6887 series instructions and ISO 11290-2:2017 or</li> <li>Add one sponge to 100 mL Oxoid™ 24 LEB (without selective supplement) with 4.4 mL of Oxoid™ 24 LEB Buffer Supplement<sup>[1]</sup></li> </ul>

<sup>[1]</sup> 24 LEB Buffer Supplement may crystallize during storage. If crystals are present, place the tube in a 37°C water bath for 5–10 minutes, or until all of the crystals are dissolved.

- Gently agitate the bag, then transfer 100 µL onto one Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) plate or transfer 1 mL of the enrichment onto three Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) plates. Alternatively, transfer 1 mL of sample preparation into a 90 mm sterile petri dish and pour 20±2 mL of molten (45±1°C) Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) into the petri dish.
- Repeat this step for each dilution.
- Incubate the plates at 37±1°C for 24–48 hours ± 2 hours. The plates can be read in 22 hours.

**Note:** It is possible to store the plates after incubation for 72 hours at 5°C±3°C before reading.

*Listeria* species colonies grow as blue-green colonies. *Listeria monocytogenes* colonies will include the addition of a typical halo. Non-target organisms are either inhibited or grow as straw or white colonies.

---


**Note:** Some *L. ivanovii* strains can as well show a typical halo due to a positive lecithinase activity, but these halos are smaller than the halos around *L. monocytogenes* colonies.

---

Blue-green colonies are presumptive positive *Listeria* species, and blue-green colonies with halos are presumptive positive *L. monocytogenes*.

See “Confirm positive results” to confirm the observed characteristic colonies.

## Listeria *Precis*™ Enumeration Method workflow

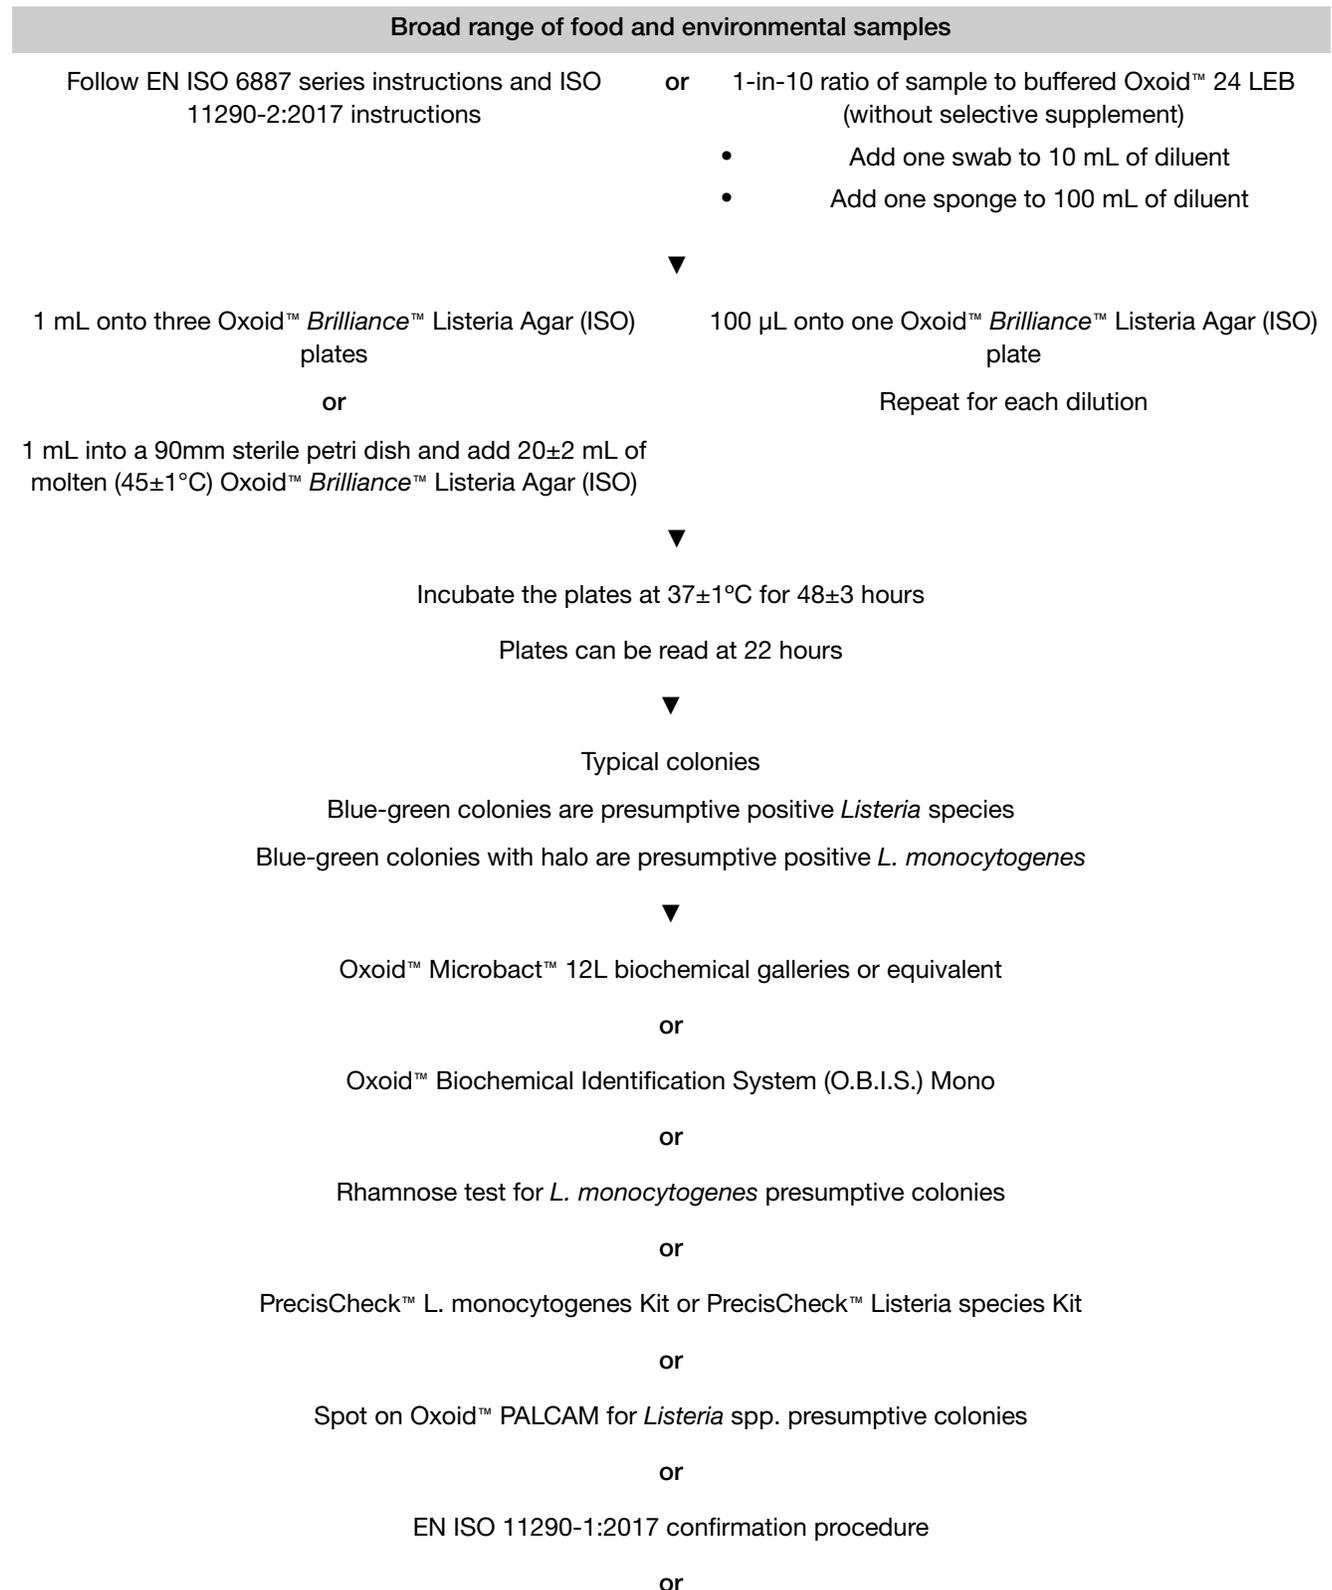

(continued)

**Broad range of food and environmental samples**

Molecular hybridization test as described in EN ISO 7218:2007 (e.g. SureTect™ *Listeria* species PCR Assay and/or SureTect™ *Listeria monocytogenes* PCR Assay)

or

Any appropriate EN ISO 16140-6:2019 validated confirmation method

## Example results

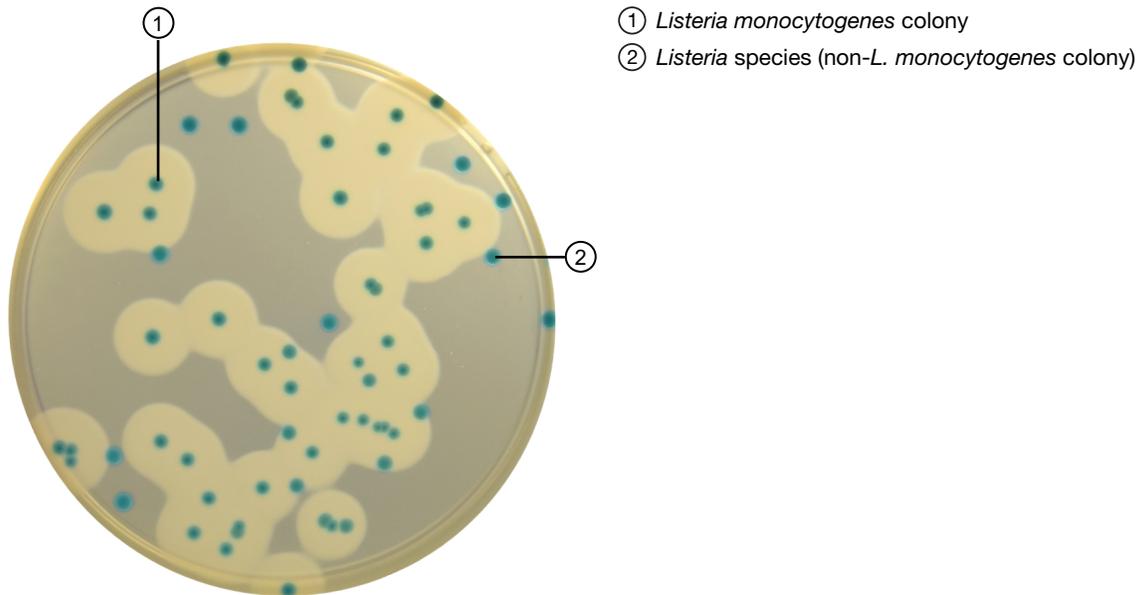


Figure 1 Example results—mixed culture

## Confirm positive results

In the context of NF VALIDATION™, all samples identified as presumptive for *Listeria* species and/or *L. monocytogenes* shall be confirmed.

Confirmation is performed from isolated characteristic colonies on Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) and running one of these four options:

- Option 1: *PrecisCheck*™ *L. monocytogenes* Kit (Cat. No. [LF0200A](#)) or *PrecisCheck*™ *Listeria* species Kit (Cat. No. [LF0100A](#)) (pick depending on colony characteristic). See Appendix A, “Confirmation of presumptive colonies using *PrecisCheck*™ *Listeria* Kits” for more details.
- Option 2: Biochemical galleries, e.g. Oxoid™ *Microbact*™ *Listeria* 12L Kit (Cat. No. [MB1128A](#)).
- Option 3: Oxoid™ Biochemical Identification System (O.B.I.S.) Mono (Cat. No. [ID0600M](#)) that rapidly differentiates *Listeria monocytogenes* from other *Listeria* species in 6 minutes.
- Option 4: Perform a Rhamnose test according to ISO 11290:2017 part 1 and part 2 standards. In most cases (particularly for microvolume tubes), positive reactions indicated by a color usually occur within 24–48 hours, but can take up to 5 days.

In the context of ISO general rules, it is as well possible to confirm the colonies with one of the following options:

1. Any appropriate EN ISO 16140-6:2019 validated method.
2. EN ISO 11290:2017 confirmation procedure.
3. Molecular hybridization as described in EN ISO 7218:2007 using for instance the *SureTect*™ *Listeria* species PCR Assay [A56842](#) and *SureTect*™ *Listeria monocytogenes* PCR Assay (Cat. No. [A56843](#)) that are validated according to the ISO 16140-2:2016 standard (respectively NF VALIDATION™ certificate UNI 03/08-11/13 and NF VALIDATION™ certificate UNI 03/09-11/13).

In the event of discordant results (positive with the *Listeria* *Precis*™ Methods or non-confirmed by one of the means described above), the laboratory must follow the necessary steps to ensure the validity of the result obtained.

## Performance validation

Table 12 NF VALIDATION™ certification of the methods

Certification	Scope and expiration
 <p>ALTERNATIVE ANALYTICAL METHODS FOR AGRIBUSINESS <a href="http://nf-validation.afnor.org/en">http://nf-validation.afnor.org/en</a></p>	<p>The NF VALIDATION™ certificate can be obtained from our Technical Support team</p> <ul style="list-style-type: none"><li>• (Europe: email: <a href="mailto:microbiology.techsupport.uk@thermofisher.com">microbiology.techsupport.uk@thermofisher.com</a> telephone: +44 (0)1256 694238)</li><li>• AFNOR Certification (<a href="http://nf-validation.afnor.org/en">nf-validation.afnor.org/en</a>)</li></ul> <p>For more information about the validity of the NF VALIDATION™ certification, please refer to the certificates UNI 03/04-04/05 and UNI 03/14-06/22 for the detection method and UNI 03/04-09/06 for the enumeration method available at <a href="http://nf-validation.afnor.org/en">nf-validation.afnor.org/en</a> or obtain from our technical support team.</p>

## Appendix A Confirmation of presumptive colonies using PrecisCheck™ *Listeria* Kits

### PrecisCheck™ *L. monocytogenes* Kit (Cat. No. LF0200A)

Confirmation is performed from isolated characteristic colonies on Oxoid™ *Brilliance*™ *Listeria* Agar (ISO):

1. Select 1 to 5 isolated presumptive colonies on the Oxoid™ *Brilliance*™ *Listeria* Agar (ISO) plate.
2. Emulsify the colony (or colonies) in 300 µL of diluent (e.g. saline, BPW) inside a cluster tube.
3. Place the PrecisCheck™ *L. monocytogenes* test strip into inoculated cluster tube with the arrow facing down.
4. Incubate for 20 minutes. Although some reactions may take up to 20 minutes, it is possible to obtain a positive result in 10 minutes.
5. Read the results as shown in Figure 2.

## PrecisCheck™ *Listeria* species Kit (Cat. No. LF0100A)

Confirmation is performed from isolated characteristic colonies on Oxoid™ *Brilliance™* *Listeria* Agar (ISO):

1. Select 1 to 5 isolated presumptive colonies on the Oxoid™ *Brilliance™* *Listeria* Agar (ISO) plate.
2. Emulsify the colony (or colonies) in 300 µL of diluent (e.g. saline, BPW) inside a cluster tube.
3. Heat for 5 to 15 minutes at 95–100°C (using a dry bath incubator or equivalent).
4. Cool to room temperature.
5. Place the PrecisCheck™ *Listeria* species test strip into inoculated, heat-treated, cluster tube with the arrow facing down.
6. Incubate for 20 minutes. Although some reactions may take up to 20 minutes, it is possible to obtain a positive result in 10 minutes.
7. Read the results as shown in Figure 2.

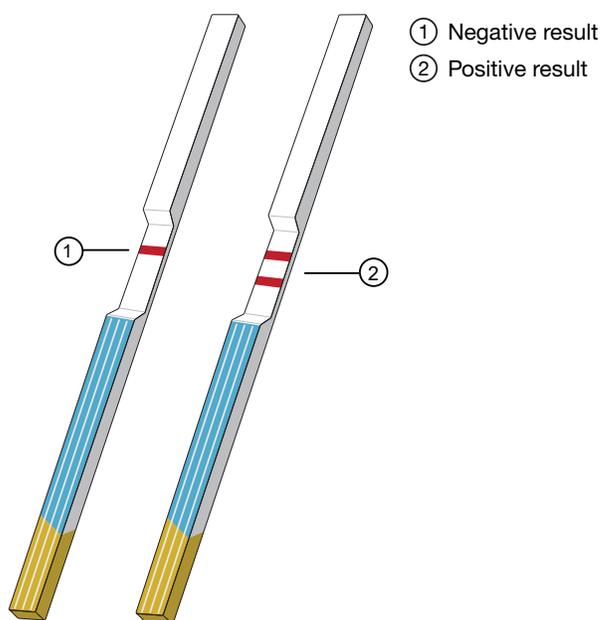


Figure 2 PrecisCheck™ *Listeria* test strip results

- No color line: the quality control is negative; something went wrong; repeat the test.
- One single color line: the quality control assesses the validity of the test and the result is negative.
- Two color lines: the quality control assesses the validity of the test and the result is positive.

---

## References

- EN ISO 7218:2007. Microbiology of food and animal feeding stuffs— General requirements and guidance for microbiological examinations.
- EN ISO 6887-1:2017. Microbiology of the food chain— Preparation of test samples, initial suspension and decimal dilutions for microbiological examination— Part 1: General rules for the preparation of the initial suspension and decimal dilutions.
- EN ISO 6887-2:2017. Microbiology of the food chain— Preparation of test samples, initial suspension and decimal dilutions for microbiological examination— Part 2: Specific rules for the preparation of meat and meat products.
- EN ISO 6887-4:2017. Microbiology of the food chain— Preparation of test samples, initial suspension and decimal dilutions for microbiological examination— Part 4: Specific rules for the preparation of miscellaneous products.
- ISO 6887-3:2017. Microbiology of the food chain— Preparation of test samples, initial suspension and decimal dilutions for microbiological examination— Part 3: Specific rules for the preparation of fish and fishery products.
- EN ISO 6887-5:2020. Microbiology of the food chain— Preparation of test samples, initial suspension and decimal dilutions for microbiological examination— Part 5: Specific rules for the preparation of milk and milk products.
- ISO 11290:1-2017. Microbiology of the food chain— Horizontal method for the detection and enumeration of *Listeria monocytogenes* and of *Listeria* spp.— Part 1: Detection method.
- ISO 11290:2-2017. Microbiology of the food chain— Horizontal method for the detection and enumeration of *Listeria monocytogenes* and of *Listeria* spp.— Part 2: Enumeration method.
- EN ISO 16140-2:2016. Microbiology of food and animal feed— Method validation— Part 2: Protocol for the validation of alternative (proprietary) methods against a reference method.
- EN ISO 16140-6:2019. Microbiology of food and animal feed— Method validation— Part 6: Protocol for the validation of alternative (proprietary) methods for microbiological confirmation and typing procedures.
- FDA *Bacteriological Analytical Manual* (BAM), Chapter 10: Detection of *Listeria monocytogenes* in Foods and Environmental Samples and Enumeration of *Listeria monocytogenes* in Foods.
- Ottaviani F., Ottaviani M., Agosti M., Differential agar medium for *Listeria monocytogenes*. Quimper Froid Symposium Proceedings, P6 ADRIA Quimper, France, 16–18 June 1997.
- Ottaviani F., Ottaviani M., Agosti M., Esperienza su un agar selettivo e differenziale per *L. mono*. Industrie Alimentari, 1997.
- USDA/FSIS *Microbiology Laboratory Guidebook* (MLG) 8.13 Isolation and Identification of *Listeria monocytogenes* from Red Meat, Poultry, Ready-To-Eat Siluriformes (Fish) and Egg Products, and Environmental Samples.

Revision history: MAN0026538 G (English)

Revision	Date	Description
G	19 November 2024	A revision was made concerning the Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Buffer Supplement. The AFNOR validation was not affected.
F	18 October 2024	A footnote was added for the Oxoid™ 24 Listeria Enrichment Broth (24 LEB) Buffer Supplement.
E	30 July 2024	Instructions were added for preparing Oxoid™ 24 LEB Complete.
D00	21 March 2024	A footnote was added for 24 Listeria Enrichment Broth (24 LEB) (10 × 225 mL in 250 mL PET sirop bottles).
C.0	23 October 2023	Instructions were added for preparing Oxoid™ <i>Brilliance</i> ™ Listeria Agar (ISO) Bottle Media.
B.0	22 May 2023	An amendment was made to the confirmation section.
A.0	12 January 2023	New document created for NF VALIDATION™ study of Thermo Scientific™ Listeria PreciS™ Methods.

The information in this guide is subject to change without notice.

**DISCLAIMER:** TO THE EXTENT ALLOWED BY LAW, THERMO FISHER SCIENTIFIC INC. AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Limited Use Label License: This product or portions hereof are subject to proprietary rights of Epoch Biosciences, Inc. and are made and sold under license from Epoch under the patents and patent applications as may be designated by Epoch from time to time set forth, including one or more of the following: U.S. Patent Nos. 6,699,975, 7,718,374, 7,348,146 and 7,671,218, and related U.S. and foreign patents and pending applications. A license must be obtained directly from Epoch with respect to any other proposed use of this product.

Buyer agrees and understands it is not licensed to (a) provide commercial data or databases to or on behalf of any third party that relate to use of the product; or (b) use the product or data there from in a clinical diagnostic setting where data from an individual's sample is given to such individual or their caregiver. Neither Epoch Biosciences nor its licensors grants any other licenses, express or implied, to permit the manufacture, use, sale, or importation of the product, any other nucleic acids, or any data generated from use of the product.

Trademarks: All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. AFNOR and NF VALIDATION are trademarks of Association Française de Normalisation (AFNOR).

©2023-2024 Thermo Fisher Scientific Inc. All rights reserved.