

Performance characteristics, continued

Expected values

This assay was tested with human serum, and plasma samples at dilutions from 1:10 to 1:60 in Assay Buffer.

Sample	Range (mg/dL)	Average (mg/dL)
Human serum/plasma [1]	36.7–246.7	104.0

[1] The normal reference range for adults is 70–105 mg/dL.

Sensitivity

The analytical sensitivity of the assay is 0.413 mg/dL glucose. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 20 times, and calculating the corresponding concentration.

Linearity of dilution

Linearity was determined by assaying human serum and plasma samples with high and low concentrations of glucose (high sample 10.7 mg/dL; low sample 3.67 mg/dL) mixed in the ratios shown in the following table.

Low Sample %	High Sample %	Expected Conc. (mg/dL)	Observed Conc. (mg/dL)	% Recovery
Serum samples				
80	20	5.09	4.61	90.6
60	40	6.51	6.49	99.8
40	60	7.93	7.79	98.3
20	80	9.35	9.26	99.0
Mean Recovery				96.9%

Plasma samples				
80	20	2.89	2.69	93.2
60	40	3.52	3.68	104.4
40	60	4.15	4.05	97.5
20	80	4.79	5.10	106.6
Mean Recovery				100.4%

Glucose Colorimetric Detection Kit

Catalog Number EIAGLUC (192 tests)

Rev 1.0

For safety and biohazard guidelines, see the “Safety” appendix in the *ELISA Technical Guide* (Pub. no. MAN0006706). Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves.

Product description

The Glucose Colorimetric Detection Kit is designed to measure glucose in serum, plasma, urine, buffered solutions, and tissue culture medium. The kit uses glucose oxidase to react with glucose to produce hydrogen peroxide which, in the presence of horseradish peroxidase, reacts with a colorless substrate to produce a colored product. The assay was characterized with human samples, but can be used to test samples from other species.

Glucose is the most common carbohydrate. It is a hexose sugar that is also known as dextrose, because it is dextrorotatory. Glucose is produced from the breakdown of glycogen, and also synthesized in the liver and kidneys through the process of gluconeogenesis.

Contents and storage

Kit and components are shipped at –20°C. Upon receipt, store the kit at –20°C. Once open, store the kit at 4°C and use within 2 weeks.

Components	Quantity
Glucose Standard; 320 mg/dL glucose in a special stabilizing solution	90 µL
Clear 96-well Half Area Plate	2 plates
Assay Buffer; contains detergent and stabilizers	50 mL
Substrate	5 mL
Horseradish Peroxidase Concentrate; 100X HRP in a special stabilizing solution	60 µL
Glucose Oxidase Concentrate; 10X glucose oxidase in a special stabilizing solution	600 µL

Materials required but not supplied

- Microtiter plate reader with software capable of measurement at or near 560 nm
- Calibrated adjustable precision pipettes and glass or plastic tubes for diluting solution

Procedural guidelines

Reagents are lot-specific. Do not mix or interchange different reagent lots from various kit lots.

Sample preparation guidelines

- Collect samples in pyrogen/endotoxin-free tubes.
- Freeze samples after collection if samples will not be tested immediately. Avoid multiple freeze-thaw cycles of frozen samples. Thaw completely and mix well (do not vortex) prior to analysis.
- If large amounts of particulate matter are present in the sample, centrifuge or filter sample prior to analysis.

Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at www.thermofisher.com/us/en/home/global/terms-and-conditions.html. If you have any questions, please contact Life Technologies at www.thermofisher.com/support.

 Catalog Number
  Batch code
  Temperature limitation
  Use by
  Manufacturer
  Consult instructions for use
  Caution, consult accompanying documents

Manufacturer's address: Life Technologies Corporation | 7335 Executive Way | Frederick, MD 21704 | USA

The information in this guide is subject to change without notice.

DISCLAIMER

TO THE EXTENT ALLOWED BY LAW, LIFE TECHNOLOGIES AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Important Licensing Information: These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

Corporate entity: Life Technologies Corporation | Carlsbad, CA 92008 USA | Toll Free in USA 1 800 955 6288

© 2017 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. Triton is a trademark of Dow Chemical Company. Tween is a trademark of Croda Americas.

For support visit thermofisher.com/support or email techsupport@lifetech.com.

thermofisher.com

17 February 2017



For research use only. Not for use in diagnostic procedures.



Dilute samples


Sample concentrations should be within the range of the standard curve. Because conditions may vary, each investigator should determine the optimal dilution for each application.

- Dilute **serum** and **plasma** samples ≥1:15 in Assay Buffer.
- Dilute **urine** samples ≥1:2 in Assay Buffer.
- Perform sample dilutions with Assay Buffer.
- Use all samples within **2 hours** of dilution.

Dilute standards

Note: Use glass or plastic tubes for diluting standards.

1. Briefly vortex the vial of standard to ensure the contents are mixed.
2. Add 15 µL Glucose Standard to one tube containing 135 µL Assay Buffer and label as 32 mg/dL glucose.
3. Add 75 µL Assay Buffer to each of 7 tubes labeled as follows: 16, 8, 4, 2, 1, 0.5, and 0 mg/dL glucose.
4. Make serial dilutions of the standard as described below in the dilution diagram. Mix thoroughly between steps.
5. **Use the standards within 2 hours of preparation.**

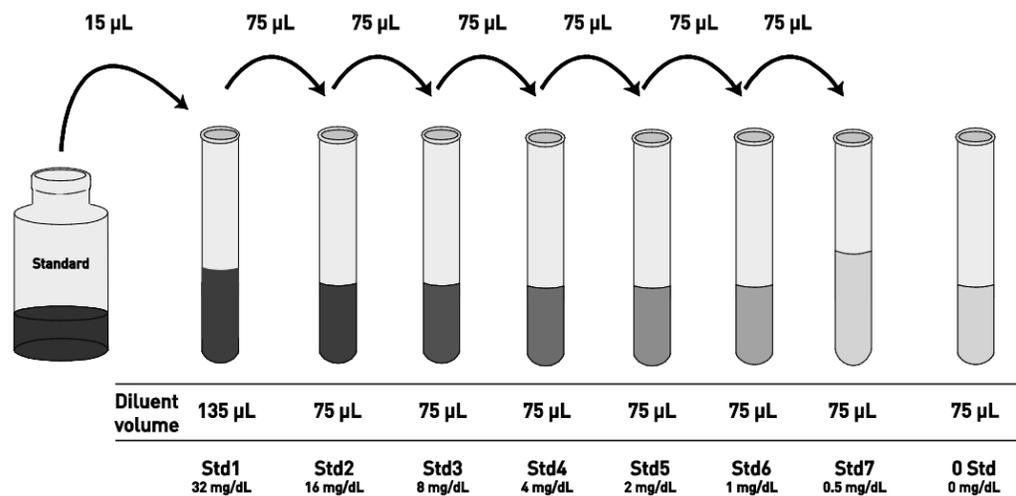

Prepare 1X HRP solution

Dilute Horseradish Peroxidase Concentrate (100X) 1:100 with Assay Buffer.

Reagent	½ plate	1 plate	2 plates
Horseradish Peroxidase Concentrate (100X)	15 µL	30 µL	55 µL
Assay Buffer	1.485 mL	2.97 mL	5.445 mL
Total volume	1.5 mL	3 mL	5.5 mL

Prepare 1X Glucose Oxidase


Dilute Glucose Oxidase Concentrate (10X) 1:10 with Assay Buffer.

Reagent	½ plate	1 plate	2 plates
Glucose Oxidase Concentrate (10X)	150 µL	275 µL	550 µL
Assay Buffer	1.350 mL	2.475 mL	4.95 mL
Total volume	1.5 mL	2.75 mL	5.5 mL

Assay procedure


Allow all reagents to reach room temperature before use. Mix all liquid reagents prior to use. **Total assay time is 30 minutes.**

IMPORTANT! Perform a standard curve with each assay.



Add sample and HRP solution

- Add 20 µL of standards or diluted samples (see page 2) to the appropriate wells.
- Add 25 µL 1X HRP solution into each well.



Add substrate

- Add 25 µL Substrate into each well.
- Add 25 µL 1X Glucose Oxidase into each well
- Incubate for 30 minutes at room temperature.

● Target → Horseradish peroxidase — Substrate ○ Enzyme

Read the plate and generate the standard curve

1. Read the absorbance at 560 nm.
2. Use curve-fitting software to generate the standard curve. A four parameter algorithm provides the best standard curve fit. Optimally, the background absorbance may be subtracted from all data points, including standards, unknowns and controls, prior to plotting.
3. Read the concentrations for unknown samples and controls from the standard curve. Multiply value(s) obtained for sample(s) by the appropriate factor to correct for the sample dilution.

Note: Dilute samples producing signals greater than that of the highest standard in the appropriate diluent and reanalyze. Multiply the concentration by the appropriate dilution factor.

Performance characteristics

Standard curve (example)

The following data were obtained for the various standards over the range of 0–32 mg/dL glucose.

Standard Glucose (mg/dL)	Optical Density (560 nm)
32	1.861
16	1.577
8	1.060
4	0.586
2	0.344
1	0.200
0.5	0.155
0	0.058

Note: 100 mg/dL of glucose is equivalent to 5.51 mM glucose.

Intra-assay precision

Three human serum samples were assayed in replicates of 20 to determine precision within an assay.

Parameters	Sample 1	Sample 2	Sample 3
Mean (mg/dL)	13.96	9.54	1.78
%CV	41	3.4	10.5

CV = Coefficient of Variation

Inter-assay precision

Three human serum samples were assayed 17 times in duplicate by three operators to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (mg/dL)	13.19	9.40	1.59
%CV	11.2	6.4	9.4

CV = Coefficient of Variation